


PCTWORLD INTELLECTUAL PROPERTY ORGANIZATION
International Bureau

INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification ⁶ : A61N 1/36	A1	(11) International Publication Number: WO 97/26042
		(43) International Publication Date: 24 July 1997 (24.07.97)

(21) International Application Number: PCT/RU96/00311	(81) Designated States: AU, CN, CZ, JP, US, European patent (AT, BE, CH, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE).
(22) International Filing Date: 31 October 1996 (31.10.96)	
(30) Priority Data: 96100043 18 January 1996 (18.01.96) RU	Published With international search report.
(71) Applicant (for all designated States except US): OPEN JOINT-STOCK COMPANY "PLANT "KOMPOONENT" [RU/RU]; Plant Komponent Ltd., Zelenograd, Moscow, 103460 (RU).	
(72) Inventors; and (75) Inventors/Applicants (for US only): TEREKHIN, Jury Vladimirovich [RU/RU]; Zelenograd 116-36, Moscow, 103480 (RU). OUGADTCHIKOV, Anatoli Leontievich [RU/RU]; Zelenograd 1110-20, Moscow, 103460 (RU).	

(54) Title: ELECTRICAL STIMULANT FOR ALIMENTARY TRACT

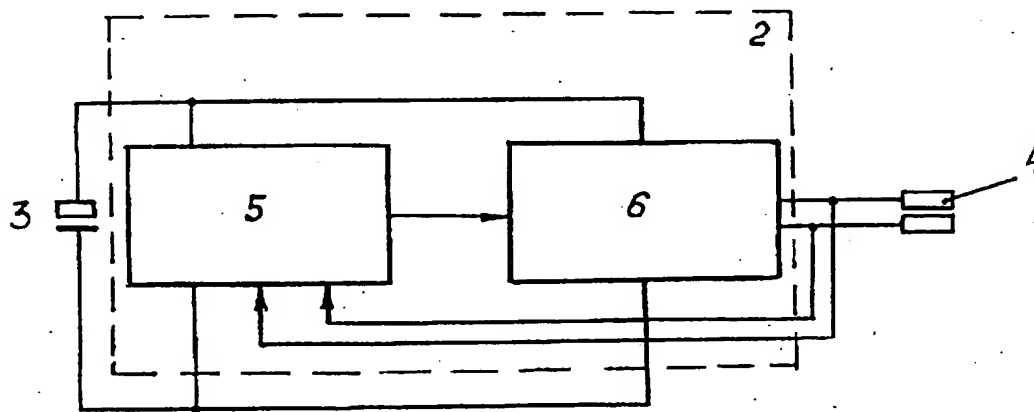

(57) Abstract

The invention relates to the medical equipment and can be used, for example, in post-surgical therapy in outpatient clinics and in hospitals, as well as prophylactic measure at alimentary tract diseases. Essence: an electrical stimulant contains capsule (1), in which consecutively connected unit (5) for testing parameters of external medium and pulses driver (6), connected to power supply (3), are located. Electrodes (4) are provided on the external surface of capsule (1), total in-number $(2 + n)$, where $n = 0, 1, 2, \dots$, and is defined by a degree of healing effect for some or other disease and technological possibility of the electrodes manufacture. Electrodes (4) are connected with the output of pulses driver (6) and also with inputs of unit (5). In case of multi-electrodes form of the electrical stimulant two electrodes only are connected both with the unit (6) and the unit (5).

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AM	Armenia	GB	United Kingdom	MW	Malawi
AT	Austria	GE	Georgia	MX	Mexico
AU	Australia	GN	Guinea	NE	Niger
BB	Barbados	GR	Greece	NL	Netherlands
BE	Belgium	HU	Hungary	NO	Norway
BF	Burkina Faso	IE	Ireland	NZ	New Zealand
BG	Bulgaria	IT	Italy	PL	Poland
BJ	Benin	JP	Japan	PT	Portugal
BR	Brazil	KE	Kenya	RO	Romania
BY	Belarus	KG	Kyrgyzstan	RU	Russian Federation
CA	Canada	KP	Democratic People's Republic of Korea	SD	Sudan
CF	Central African Republic	KR	Republic of Korea	SE	Sweden
CG	Congo	KZ	Kazakhstan	SG	Singapore
CH	Switzerland	LI	Liechtenstein	SI	Slovenia
CI	Côte d'Ivoire	LK	Sri Lanka	SK	Slovakia
CM	Cameroon	LR	Liberia	SN	Senegal
CN	China	LT	Lithuania	SZ	Swaziland
CS	Czechoslovakia	LU	Luxembourg	TD	Chad
CZ	Czech Republic	LV	Latvia	TG	Togo
DE	Germany	MC	Monaco	TJ	Tajikistan
DK	Denmark	MD	Republic of Moldova	TT	Trinidad and Tobago
EE	Estonia	MG	Madagascar	UA	Ukraine
ES	Spain	ML	Mali	UG	Uganda
FI	Finland	MN	Mongolia	US	United States of America
FR	France	MR	Mauritania	UZ	Uzbekistan
GA	Gabon			VN	Viet Nam

ELECTRICAL STIMULANT FOR ALIMENTARY TRACT

5

Technical field

This invention relates to the medicine and medical equipment and can be used in a post-surgical period for
10 rehabilitation of sick people suffered from weak functioning of internal organs, located close to the alimentary tract, as well of all parts of alimentary tract, by a method of "soft therapy" by means of per oral consumption of the electrical stimulant. The invention can be recommended also as
15 prophylactic measure at various kinds of alimentary tract diseases, for use in hospitals and outpatient clinics as well as by patients themselves according to the recommendation of a doctor.

20

Background Art

There is a problem at present all over the world of treatment and restoration of weakened various parts of the alimentary tract, and also of internal organs, functionally connected with the alimentary tract.

25

The use of a "soft therapy" by means of electrical stimulation at a qualitatively new level is one of the ways for solving this problem.

An electrical stimulant for the alimentary tract is known, which contains drainage tubes with electrodes located
30 on them (inventor's certificate SU 1389776, IPC A 61 M 25/00, A 61 B 5/04, of April 23, 1988).

This electrical stimulant can be used in hospitals only and by specially trained staff; there are some probability of patients injuries at the introduction and removal of the
35 device with all additives, including electrodes, through the

- 2 -

nasopharynx. Its efficiency may be insufficient because of narrow framework of its action.

An electrical stimulant of the alimentary tract, which is described in inventor's certificate SU 936931, IPC A 61 N 1/36 of June 23, 1982, may be considered as the nearest to the claimed invention according to the entirety of their essential features. That electrical stimulant contains a capsule with a power supply and a generator of pulses located inside. A capsule case is executed in a form of two electrically isolated parts, serving as electrodes being in the contact with the intestine walls after the capsule was swallowed.

The electrical stimulant works as follows.

The series of rectangular pulses of predetermined parameters arrive from the generator to the electrodes, which contact the intestine walls, influence them and cause response in the form of a peristalsis wave, which transports the electrical stimulant and contents of intestines to distal parts, where the process is repeated until the capsule will leave the alimentary tract by a natural way through the anus.

However the known electrical stimulant has relatively low efficiency of electrical stimulation, because the electrical field of two electrodes corresponds to morphology of muscular fabric of the alimentary tract only partially, and because there is no adaptation of the stimulation to conditions of various parts of the alimentary tract. Besides, it is characterized by inefficient power consumption that can affect operational reliability. Besides, absence of the stimulation adaptation to conditions of various parts of the alimentary tract can result in collateral actions on patient's body.

Insufficient efficiency of the electrical stimulation, caused by absence of stimulation adaptation to conditions existing in various parts of the alimentary tract is explained by that each part of the alimentary tract which is passed by the electrical stimulant has its own peculiarities:

- 3 -

- morphological features (geometrical size, direction and etc.);

- its own particular value of content's pH factor, which 5 determines a functional and physiological purpose of the given part.

The known electrical stimulant produces electrical pulses with mean parameters, which are not optimized for each part of the tract.

10 The relatively low efficiency of electrical stimulation caused by a partial adjustment of the electrical field of two electrodes with the morphology of the muscular tissue of the alimentary tract, is explained by the following. The muscular tissue contains an external longitudinal and internal circular 15 layers. The electrical effect on those layers requires availability of electrical fields having changing parameters and/or mutually orthogonal strength directions, which are not available by use of the known electrical stimulant. At the movement of the known electrical stimulant, the electrical 20 field of two electrodes stimulates basically the longitudinal muscular layer only, i.e. the peristalsis wave does not arise in this case or arises rarely and has unstable character, that reduces the efficiency of the electrical stimulation.

The low reliability of the known electrical stimulant as 25 the result of inefficient energy consumption is explained by impossibility of minimization of energy consumption in the mode of passive storage, because the known electrical stimulant has been in the condition of dynamic mode of operations constantly, since the moment of its manufacturing, 30 and further during storage, and after the introduction in the patient's alimentary tract.

Disclosure of Invention

The invention is directed to solving the following 35 problems:

- 4 -

- designing an electrical stimulant, which is provided for electrical fields having changing parameters and also electrical fields which strength direction is mutually
5 orthogonal.

- minimization the energy consumption in a mode of storage and consequently improving the reliability.

The essence of the claimed invention consists in that the electrical stimulant of the alimentary tract contains a
10 capsule with two electrodes, which are provided on the outer surface of the capsule, and the power supply located inside, wherein a unit for testing parameters of external medium and a pulses driver, which are consecutively connected, are additionally located in the capsule, and n electrodes, where n
15 $= 0, 1, 2, \dots$, and it is defined by a degree of healing effect for some or other disease and technological possibility of the electrodes manufacture, are provided on the external surface of the capsule, the electrodes being connected with outputs of the pulses driver and two electrodes being
20 connected also with inputs of the unit for testing parameters of external medium.

Besides the capsule can be made in the form of a tubular element with covers, each opposite end of the tubular element being provided by electrodes located on the cylinder surface.

25 Besides the capsule can be made in the form of two interconnected caps, each being provided by electrodes located on the generatrix surface.

So it is clear from the technical essence of the invention that the electrical stimulant may be drafted in
30 bi-electrodes form as well as in multi-electrodes one.

What about the newly introduced units, the additional use of the unit for testing parameters of external medium connected with the pulses driver and the electrodes provides for a feedback in the power supply circuit of the electrical
35 stimulant.

- 5 -

The unit for testing parameters of external medium registers the resistance between the electrodes which is near to infinity in the mode of electrical stimulant storage and 5 the output signal of the unit blocks the clock frequency which is responsible for the operation mode of the pulses driver. So, the electrical stimulant is in the non-working position with minimum energy consumption. When the electrical stimulant enters into the alimentary tract, anus or vagina, the 10 resistance is lowering down to the level of several kilo ohms (kOm) and the units' for testing parameters of external medium output signal coming to the managing (control) input of the pulses driver permits to start on the pulses driver and to pass it on to the working mode of electrical stimulation.

15 The pulses driver provides for series of pulses with required parameters depending on external medium pH factor.

A microprocessor which have stored in memory the necessary number of groups of stimulating parameters can be used as the pulses driver.

20 Two electrodes are used not only for electrical stimulation but also - in a pause between series of pulses - for measurement of the resistance between them, in bi-electrodes as well as in multi-electrodes form of the electrical stimulant.

25 In the electrical stimulant bi-electrodes form the pulses driver signals on the electrodes provide for bi-phase, orthogonal change of the electrical field vector. Parameters of the stimulating pulses can change during the electrical stimulant transportation through the alimentary tract 30 depending on the external medium pH factor.

In the electrical stimulant multi-electrodes form the pulses driver signals on the electrodes provide for multi-phase electrical field with discreteness of $n!$, where n is the number of the electrodes. In this case parameters of 35 the stimulating pulses can also change during the electrical stimulant transportation through the alimentary tract.

- 6 -

Brief Description of Drawings

The essence of the invention is explained by the drawings, where:

5 Fig.1 shows a functional electrical diagram of the electrical stimulant in bi-electrodes form.

Fig.2 represents a constructive embodiment of the electrical stimulant with the capsule designed in the form of a tubular element with covers, each opposite end of the
10 tubular element being provided by one electrode located on the cylinder line (bi-electrodes form).

Fig.3 is a constructive embodiment of the electrical stimulant with the capsule designed in the form of two interconnected caps, each being provided by the electrodes
15 located on the generatrix line of the cap (multi-electrodes form).

Fig.4 shows an electrical diagram of the unit for testing parameters of external medium, example for bi-electrodes form of the electrical stimulant.

20 Fig.5 is an electrical diagram of the pulses driver, example for multi-electrodes form of the electrical stimulant.

Electrical diagrams of fig.4 and fig.5 are the examples of possible embodiments of these blocks and, as well as the illustrating text in the description relating to them, in no
25 means may limit claims of the applicant. The applicant may be free to use another embodiment of the units represented in fig 4 and fig 5.

Best Mode for Carrying Out the Invention

30 The proposed alimentary tract electrical stimulant contains capsule 1, in which an electronic block 2 and power supply 3 are located. Electrodes 4 are provided on the external surface of capsule 1, the total number of the electrodes equals $(2 + n)$, where $n = 0, 1, 2, \dots$. The

- 7 -

electronic block 2 consists of the consecutively connected unit 5 for testing parameters of external medium and pulses driver 6.

5 The electrodes 4 in the bi-electrodes form are connected with outputs of the pulses driver 6 and with inputs of the unit 5 for testing parameters of external medium, and in multi-electrodes form, two electrodes 4 only are connected with inputs of the unit 5.

10 Capsule 1 can be made in the form of tubular element 7 with covers 8, each opposite end of the tubular element being provided by a group of electrodes 4 (not shown) located on a cylinder generatrix line. Covers 8 can be of semi-spheroid, cupola, or other form.

15 The capsule 1 can be made in the form of two interconnected caps 9, each being provided by a group of electrodes 4. Caps 9 can be of conic or other form.

Unit 5 for testing parameters of external medium can be made in the form of resistance at electrodes 4 measuring block 20 and contain voltage divider 10 connected with power supply 3 and having outputs connected with the pair of differently polarized electrodes 4, and comparator 11. The inverting input of comparator 11 is connected through resistor 12 with power supply 3, and the non-inverting input - with the output of 25 voltage divider 10.

The output of comparator 11 is the control input of pulses driver 6.

Pulses driver 6 can contain three-stable linear keys 13 providing for feeding of each electrode 4 by the signal levels 30 of "+" or "-" from power supply 3 as well as switching them off from the power supply, pulses in series distributor 14 consisting of counter 15 and coder 16 and providing for consequential connection of keys' voltage inputs to the output of counter and blocking of unused keys, controlled frequency 35 divider 17 providing for formation of a pulsing sequence from

- 8 -

necessary number of pulses in a series with repetition frequency of series close to frequency of the natural peristalsis wave, and monitoring synchronizer 18 producing 5 frequency which is necessary for formation of the required duration of stimulating pulses (6-10 ms.).

The electrical stimulant works as follows (this is an example for the multi-electrodes form as the form more complicated for the understanding of its functioning).

10 The electrical stimulant is entered, for example, into the alimentary tract of a patient per oral, i.e. by swallowing.

In the initial mode (before the entering into the alimentary tract) the electrical stimulant is in the 15 non-working position, at which the voltage from voltage divider 10 blocks pulses driver 6 through unit 5 for testing parameters of external medium.

The voltage from voltage divider 10 drops after the entering into the alimentary tract of capsule 1 due to the 20 impact of external medium (saliva, gastric juice and so on) and unit 5 for testing parameters of external medium comes to the condition permitting to start on pulses driver 6.

The series of pulses, which parameters are determined by the external medium pH factor, comes from pulses driver 6 to 25 electrodes 4. Thus pulses driver 6 executes such commutation of electrodes 4 for each series of pulses, which commutation provides for activating, for example, simultaneously, pairs of differently polarized electrodes from the same group as well as from the electrodes from the opposite groups. Such 30 activation of the pairs of electrodes with mutually orthogonal electrical field strength directions provides for simultaneous or consecutive excitation the longitudinal as well as circular layers of muscular tissue irrespective of capsule orientation in any part of the alimentary tract, that increases 35 essentially electrical stimulating efficiency. The electrical

- 9 -

impact on the muscular tissue causes response in the form of the stable peristalsis wave which transports the electrical stimulant and contents, for example, of the alimentary tract, 5 to its distal part which is influenced by the next series of pulses and the process is repeated until the capsule will come out by the natural way.

- 10 -

5

CLAIMS:

1. An electrical stimulant of the alimentary tract containing a capsule with two electrodes, which are provided on the outer surface of the capsule, and the power supply 10 located inside, characterized by that a unit for testing parameters of external medium and a pulses driver, which are consecutively connected, are additionally located in the capsule, and n electrodes, where $n = 0, 1, 2, \dots$, and it is defined by a degree of healing effect for some or other 15 disease and technological possibility of the electrodes manufacture, are provided on the external surface of the capsule, the electrodes being connected with outputs of the pulses driver and two electrodes of the total number of the electrodes are connected with inputs of the unit for testing 20 of parameters of external medium.

2. The electrical stimulant of the alimentary tract according to the claim 1, characterized by that the capsule is made in the form of a tubular element with covers, each 25 opposite end of the tubular element being provided by a group of electrodes located on the cylinder generatrix line.

3. The electrical stimulant of the alimentary tract according to the claim 1, characterized by that the capsule is 30 made in the form of two interconnected caps, each being provided by a group of electrodes located on the generatrix line of the cap.

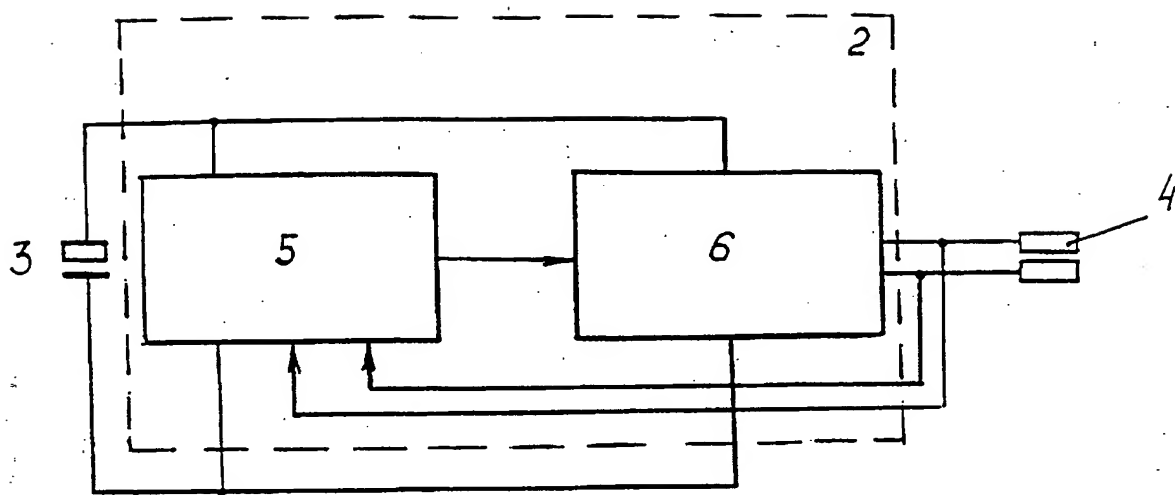


Fig.1

2/4

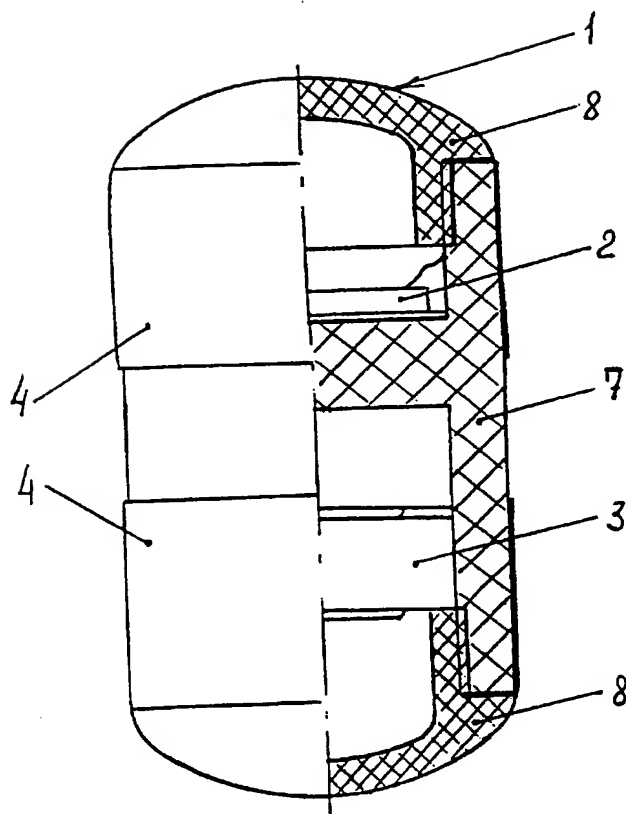


Fig.2

3/4

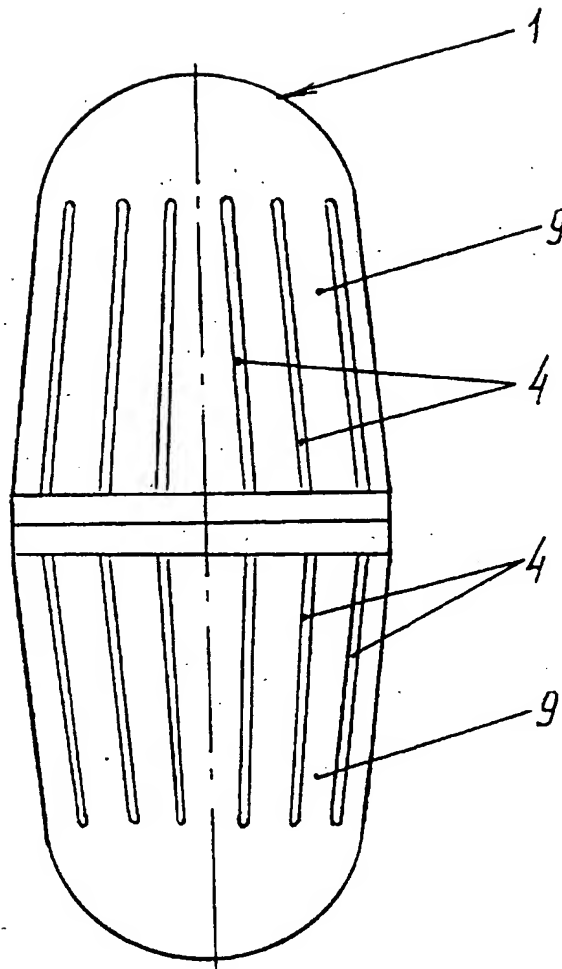


Fig.3

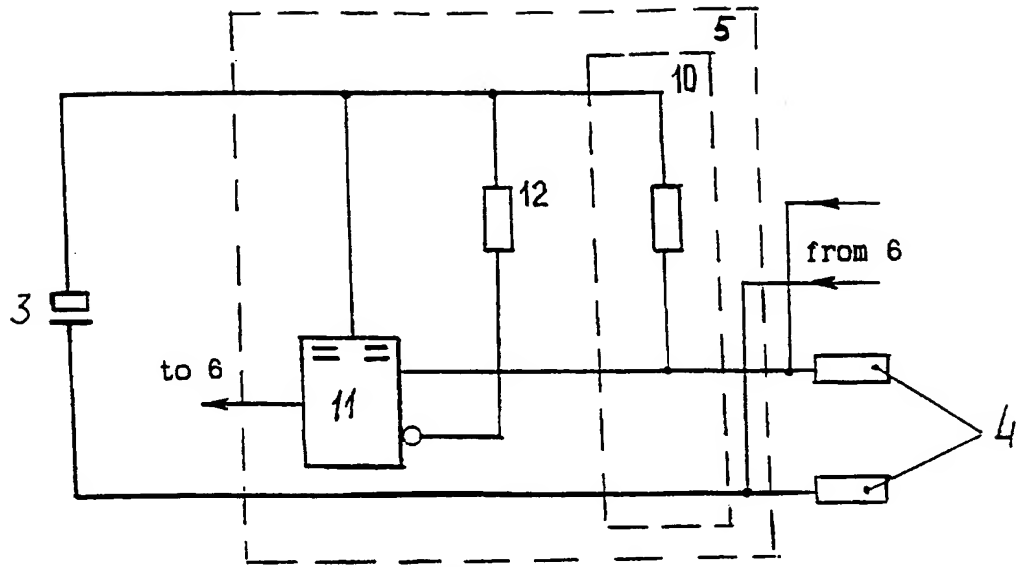


Fig.4

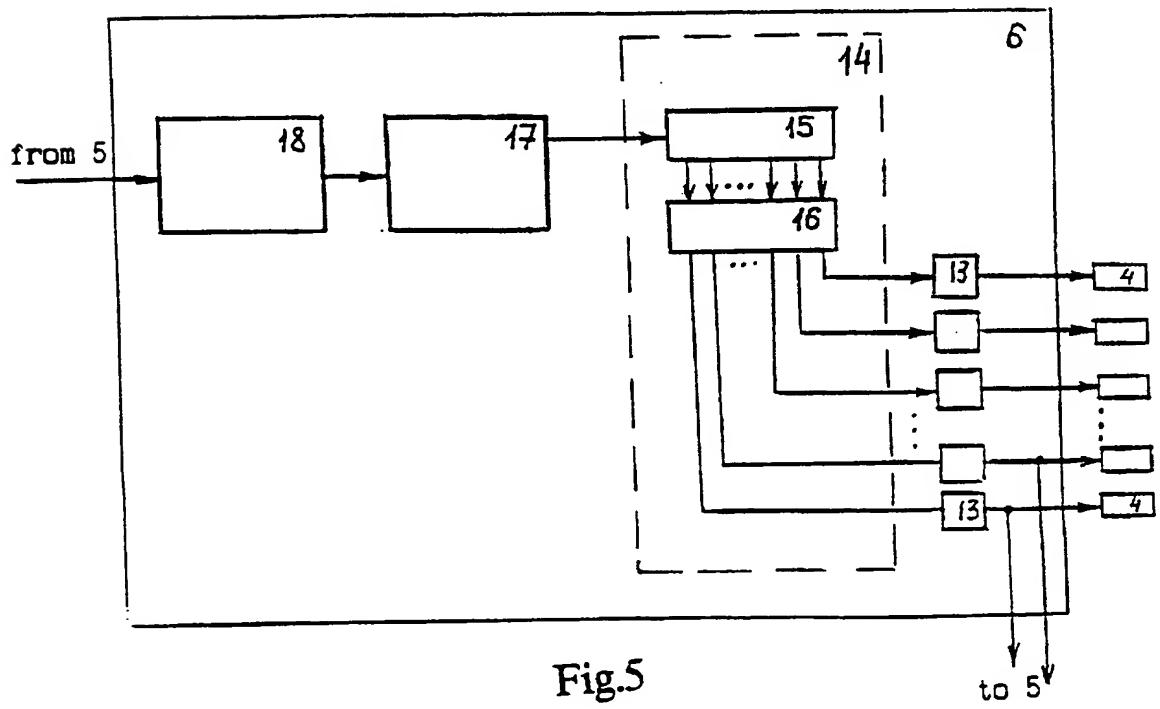


Fig.5

INTERNATIONAL SEARCH REPORT

Int. l. Application No
PCT/RU 96/00311

A. CLASSIFICATION OF SUBJECT MATTER

IPC 6 A61N1/36

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 6 A61N A61B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	WO 88 00449 A (C.B.BIOELETTRONICA) 28 January 1988 see the whole document ---	1
A	WO 94 01172 A (DOUGLAS) 20 January 1994 see the whole document ---	1
A	EP 0 193 251 A (CORNING GLASS WORKS) 3 September 1986 see abstract ---	1
A	US 3 719 183 A (SCHWARTZ) 6 March 1973 see the whole document ---	1
A	US 5 358 514 A (SCHULMAN) 25 October 1994 see the whole document ---	1
-/--		

☒ Further documents are listed in the continuation of box C.

☒ Patent family members are listed in annex.

* Special categories of cited documents :

- "A" document defining the general state of the art which is not considered to be of particular relevance
- "E" earlier document but published on or after the international filing date
- "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- "O" document referring to an oral disclosure, use, exhibition or other means
- "P" document published prior to the international filing date but later than the priority date claimed

- "T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- "X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- "Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
- "&" document member of the same patent family

Date of the actual completion of the international search

11 April 1997

Date of mailing of the international search report

18. 04. 97

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+ 31-70) 340-2040, Tx. 31 651 epo nl,
Fax (+ 31-70) 340-3016

Authorized officer

Taccoen, J-F

INTERNATIONAL SEARCH REPORT

Int. onal Application No
PCT/RU 96/00311

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT		
Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 5 209 238 A (SUNDHAR) 11 May 1993 see the whole document -----	1

1

INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No

PCT/RU 96/00311

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
WO 8800449 A	28-01-88	DE 3779895 A EP 0274499 A	23-07-92 20-07-88
WO 9401172 A	20-01-94	US 5292344 A AU 662076 B AU 4666993 A CA 2138792 A EP 0656796 A JP 7508662 T	08-03-94 17-08-95 31-01-94 20-01-94 14-06-95 28-09-95
EP 0193251 A	03-09-86	GB 2096825 A EP 0063455 A US 4502938 A US 4567006 A	20-10-82 27-10-82 05-03-85 28-01-86
US 3719183 A	06-03-73	NONE	
US 5358514 A	25-10-94	US 5405367 A US 5193540 A	11-04-95 16-03-93
US 5209238 A	11-05-93	WO 9423653 A AU 4284493 A	27-10-94 08-11-94

THIS PAGE BLANK (USPTO)